

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	03089	Calib. Date:	09/26/2025
Certification File No.:	03090	Cert. No.:	00054
Linearity File No.:	03091	Cert. Date:	09/26/2025
Solution File No.:	03151	Lin. Date:	09/26/2025
Sequential File No.:	03151	Lin. No.:	00049
		Soln. Date:	02/20/2026
		Soln. No.:	00429
		File Date:	02/20/2026
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0008
Solution Control Lot:	24370	Expires:	10/08/2026
		Bottle No.:	0898

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:34S		
Control 1 EC	0.100%	08:34S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:35S		
Control 2 EC	0.100%	08:36S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:36S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:37S		
Control 3 EC	0.099%	08:38S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:39S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JONES

First Name: CRAIG

MI: D

Signature: _____

Sgt. Jones #377

Badge No.: 377

Date: 02/20/2026

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	03089	Calib. Date: 09/26/2025
Certification File No.:	03090	Calib. No.: 00054
Linearity File No.:	03091	Cert. Date: 09/26/2025
Solution File No.:	03130	Lin. No.: 00048
Sequential File No.:	03130	Lin. Date: 09/26/2025
		Soln. No.: 00427
		Soln. Date: 12/29/2025
		File Date: 12/29/2025
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	24370	Expires: 10/08/2026
		Bottle No.: 0891

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:15S		
Control 1 EC	0.100%	10:16S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:16S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:17S		
Control 2 EC	0.098%	10:18S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:18S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:19S		
Control 3 EC	0.099%	10:19S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____

J. Watts 351

Badge No.: 351

Date: 12/29/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	03089	Calib. Date: 09/26/2025
Certification File No.:	03090	Calib. No.: 00054
Linearity File No.:	03091	Cert. Date: 09/26/2025
Solution File No.:	03118	Cert. No.: 00048
Sequential File No.:	03118	Lin. Date: 09/26/2025
		Lin. No.: 00049
		Soln. Date: 12/04/2025
		Soln. No.: 00426
		File Date: 12/04/2025
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	24370	Expires: 10/08/2026
		Bottle No.: 0892

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:38S		
Control 1 EC	0.100%	08:38S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:39S		
Control 2 EC	0.099%	08:40S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:40S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:41S		
Control 3 EC	0.099%	08:41S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:41S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

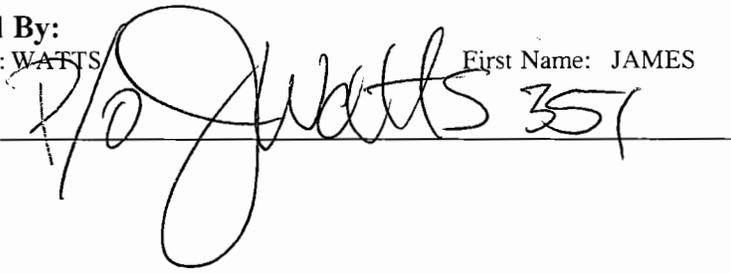
Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____



Badge No.: 351

Date: 12/04/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	03089	Calib. Date: 09/26/2025
Certification File No.:	03090	Calib. No.: 00054
Linearity File No.:	03091	Cert. Date: 09/26/2025
Solution File No.:	03108	Cert. No.: 00048
Sequential File No.:	03108	Lin. Date: 09/26/2025
		Lin. No.: 00049
		Soln. Date: 11/13/2025
		Soln. No.: 00425
		File Date: 11/13/2025
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	24370	Expires: 10/08/2026
		Bottle No.: 0895

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:03S		
Control 1 EC	0.100%	13:04S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	13:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:04S		
Control 2 EC	0.100%	13:05S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:06S		
Control 3 EC	0.099%	13:07S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:07S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____

Badge No.: 351

Date: 11/13/2025

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	03089	Calib. Date: 09/26/2025
Certification File No.:	03090	Calib. No.: 00054
Linearity File No.:	03091	Cert. Date: 09/26/2025
Solution File No.:	03100	Lin. No.: 00048
Sequential File No.:	03100	Lin. Date: 09/26/2025
		Soln. No.: 00429
		Soln. Date: 10/22/2025
		File Date: 10/22/2025
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	24370	Expires: 10/08/2026
		Bottle No.: 0686

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:43D		
Control 1 EC	0.099%	10:44D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:44D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:45D		
Control 2 EC	0.098%	10:45D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:46D		
Control 3 EC	0.098%	10:47D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:47D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____



Badge No.: 351

Date: 10/22/2025

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 03055 Calib. Date: 06/06/2025 Calib. No.: 00053
Certification File No.: 03056 Cert. Date: 06/06/2025 Cert. No.: 00047
Linearity File No.: 03057 Lin. Date: 06/06/2025 Lin. No.: 00048
Solution File No.: 03080 Soln. Date: 08/18/2025 Soln. No.: 00421
Sequential File No.: 03080 File Date: 08/18/2025

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0007
Control Solution %: 0.100% Expires: 10/08/2026
Solution Control Lot: 24370 Bottle No.: 0912

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:38D		
Control 1 EC	0.099%	12:39D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:40D		
Control 2 EC	0.099%	12:41D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:41D		
Control 3 EC	0.099%	12:42D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:43D		

All tests within acceptable tolerance.

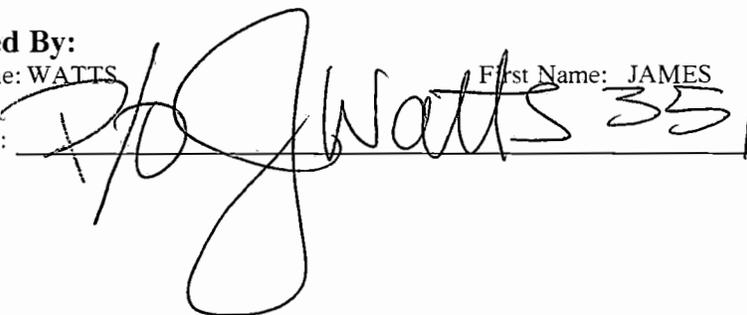
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: 

Badge No.: 351

Date: 08/18/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	03055	Calib. Date:	06/06/2025
Certification File No.:	03056	Cert. Date:	06/06/2025
Linearity File No.:	03057	Lin. Date:	06/06/2025
Solution File No.:	03071	Soln. Date:	07/24/2025
Sequential File No.:	03071	File Date:	07/24/2025
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0007
Solution Control Lot:	24370	Expires:	10/08/2026
		Bottle No.:	0904

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:21D		
Control 1 EC	0.100%	09:22D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:23D		
Control 2 EC	0.099%	09:23D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:23D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:24D		
Control 3 EC	0.099%	09:25D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____

Badge No.: 351

Date: 07/24/2025

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 03055 Calib. Date: 06/06/2025 Calib. No.: 00053
Certification File No.: 03056 Cert. Date: 06/06/2025 Cert. No.: 00047
Linearity File No.: 03057 Lin. Date: 06/06/2025 Lin.-No.: 00048
Solution File No.: 03064 Soln. Date: 06/30/2025 Soln. No.: 00419
Sequential File No.: 03064 File Date: 06/30/2025

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0007
Control Solution %: 0.100% Expires: 10/08/2026
Solution Control Lot: 24370 Bottle No.: 0905

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:14D		
Control 1 EC	0.099%	10:15D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16D		
Control 2 EC	0.100%	10:17D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:17D		
Control 3 EC	0.099%	10:18D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____



Badge No.: 351

Date: 06/30/2025

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	03055	Calib. Date: 06/06/2025
Certification File No.:	03056	Calib. No.: 00053
Linearity File No.:	03057	Cert. Date: 06/06/2025
Solution File No.:	03058	Cert. No.: 00047
Sequential File No.:	03058	Lin. Date: 06/06/2025
		Lin. No.: 00048
		Soln. Date: 06/06/2025
		Soln. No.: 00418
		File Date: 06/06/2025

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWA S3-0007
Control Solution %:	0.100%		Expires: 10/08/2026
Solution Control Lot:	24370		Bottle No.: 0896

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:56D		
Control 1 EC	0.101%	12:57D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:58D		
Control 2 EC	0.099%	12:58D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:59D		
Control 3 EC	0.099%	13:00D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUJ P2-158 584

Changed By:

Last Name: HALL First Name: JOSHUA MI: B

Signature:  Badge No.: 7750
Date: 06/06/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	Calib. Date:	01/24/2025
Calibration File No.:	03012	Calib. No.:	00052
Certification File No.:	03013	Cert. Date:	01/24/2025
Linearity File No.:	03014	Lin. Date:	01/24/2025
Solution File No.:	03048	Soln. Date:	05/19/2025
Sequential File No.:	03048	File Date:	05/19/2025
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0007
Solution Control Lot:	24370	Expires:	10/08/2026
		Bottle No.:	0901

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:20D		
Control 1 EC	0.098%	09:21D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:21D		
Control 2 EC	0.098%	09:22D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:23D		
Control 3 EC	0.099%	09:24D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____



351

Badge No.: 351

Date: 05/19/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	03012	Calib. Date: 01/24/2025
Certification File No.:	03013	Calib. No.: 00052
Linearity File No.:	03014	Cert. Date: 01/24/2025
Solution File No.:	03042	Cert. No.: 00046
Sequential File No.:	03042	Lin. Date: 01/24/2025
		Lin. No.: 00047
		Soln. Date: 04/23/2025
		Soln. No.: 00416
		File Date: 04/23/2025

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWA S3-0007
Control Solution %:	0.100%		Expires: 10/08/2026
Solution Control Lot:	24370		Bottle No.: 0911

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:01D		
Control 1 EC	0.099%	09:01D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:02D		
Control 2 EC	0.098%	09:03D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:04D		
Control 3 EC	0.098%	09:04D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:05D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____



Badge No.: 351

Date: 04/23/2025

Calibrating Unit New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location: CHERRY HILL TWSP, P.D.	
Calibration File No.: 03012	Calib. Date: 01/24/2025
Certification File No.: 03013	Cert. No.: 00052
Linearity File No.: 03014	Cert. Date: 01/24/2025
Solution File No.: 03036	Lin. No.: 00047
Sequential File No.: 03036	Lin. Date: 01/24/2025
	Soln. Date: 03/27/2025
	Soln. No.: 00415
	File Date: 03/27/2025

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWA S3-0007
Control Solution %: 0.100%		Expires: 10/08/2026
Solution Control Lot: 24370		Bottle No.: 0902

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:28S		
Control 1 EC	0.099%	22:29S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	22:29S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:30S		
Control 2 EC	0.097%	22:31S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	22:31S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:32S		
Control 3 EC	0.098%	22:32S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	22:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WARREN

First Name: STEPHEN

MI: A

Signature: 

Badge No.: 386

Date: 03/27/2025

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	Calib. No.:	00052
Calibration File No.:	03012	Calib. Date:	01/24/2025
Certification File No.:	03013	Cert. Date:	01/24/2025
Linearity File No.:	03014	Lin. Date:	01/24/2025
Solution File No.:	03033	Soln. Date:	03/22/2025
Sequential File No.:	03033	File Date:	03/22/2025
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0007
Solution Control Lot:	24370	Expires:	10/08/2026
		Bottle No.:	0906

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:18S		
Control 1 EC	0.099%	12:19S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19S		
Control 2 EC	0.098%	12:20S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:20S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:21S		
Control 3 EC	0.097%	12:22S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:22S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCGLINN

First Name: SEAN

MI: M

Signature: P/O  466

Badge No.: 466

Date: 03/22/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	03012	Calib. Date: 01/24/2025
Certification File No.:	03013	Calib. No.: 00052
Linearity File No.:	03014	Cert. Date: 01/24/2025
Solution File No.:	03024	Cert. No.: 00046
Sequential File No.:	03024	Lin. Date: 01/24/2025
		Lin. No.: 00047
		Soln. Date: 02/15/2025
		Soln. No.: 00413
		File Date: 02/15/2025
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0007
Solution Control Lot:	24180	Expires: 05/14/2026
		Bottle No.: 1415

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:15S		
Control 1 EC	0.098%	13:16S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:16S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17S		
Control 2 EC	0.096%	13:17S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18S		
Control 3 EC	0.097%	13:19S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PATTON

First Name: DANIEL

MI: L

Signature: _____

Badge No.: 460

Date: 02/15/2025

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 03012 Calib. Date: 01/24/2025 Calib. No.: 00052
Certification File No.: 03013 Cert. Date: 01/24/2025 Cert. No.: 00046
Linearity File No.: 03014 Lin. Date: 01/24/2025 Lin. No.: 00047
Solution File No.: 03021 Soln. Date: 02/04/2025 Soln. No.: 00412
Sequential File No.: 03021 File Date: 02/04/2025

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0007
Control Solution %: 0.100% Expires: 05/14/2026
Solution Control Lot: 24180 Bottle No.: 1103

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:29S		
Control 1 EC	0.097%	10:30S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:30S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:31S		
Control 2 EC	0.098%	10:32S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:32S		
Control 3 EC	0.098%	10:33S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:33S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:34S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____



Badge No.: 352

Date: 02/04/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02960	Calib. Date: 09/16/2024
Certification File No.:	02961	Calib. No.: 00050
Linearity File No.:	02962	Cert. Date: 09/16/2024
Solution File No.:	03007	Cert. No.: 00044
Sequential File No.:	03007	Lin. Date: 09/16/2024
		Lin. No.: 00045
		Soln. Date: 01/18/2025
		Soln. No.: 00410
		File Date: 01/18/2025
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	24180	Expires: 05/14/2026
		Bottle No.: 0867

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:32S		
Control 1 EC	0.100%	12:32S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:33S		
Control 2 EC	0.099%	12:34S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:35S		
Control 3 EC	0.098%	12:36S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:36S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:37S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PATTON

First Name: DANIEL

MI: L

Signature: _____



Badge No.: 460

Date: 01/18/2025

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02960 Calib. Date: 09/16/2024 Calib. No.: 00050
Certification File No.: 02961 Cert. Date: 09/16/2024 Cert. No.: 00044
Linearity File No.: 02962 Lin. Date: 09/16/2024 Lin. No.: 00045
Solution File No.: 03002 Soln. Date: 01/01/2025 Soln. No.: 00409
Sequential File No.: 03002 File Date: 01/01/2025

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0008
Control Solution %: 0.100% Expires: 05/14/2026
Solution Control Lot: 24180 Bottle No.: 0785

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:06S		
Control 1 EC	0.099%	13:07S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:07S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:08S		
Control 2 EC	0.098%	13:08S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:08S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:09S		
Control 3 EC	0.098%	13:10S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:10S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: 

Badge No.: 351

Date: 01/01/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02960	Calib. Date: 09/16/2024
Certification File No.:	02961	Calib. No.: 00050
Linearity File No.:	02962	Cert. Date: 09/16/2024
Solution File No.:	02996	Cert. No.: 00044
Sequential File No.:	02996	Lin. Date: 09/16/2024
		Lin. No.: 00045
		Soln. Date: 12/08/2024
		Soln. No.: 00408
		File Date: 12/08/2024
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	24180	Expires: 05/14/2026
		Bottle No.: 1469

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:07S		
Control 1 EC	0.100%	12:07S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:07S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:08S		
Control 2 EC	0.098%	12:09S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:09S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:10S		
Control 3 EC	0.099%	12:10S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:10S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

J. J. Weist 352

Badge No.: 352

Date: 12/08/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02960 Calib. Date: 09/16/2024 Calib. No.: 00050
Certification File No.: 02961 Cert. Date: 09/16/2024 Cert. No.: 00044
Linearity File No.: 02962 Lin. Date: 09/16/2024 Lin. No.: 00045
Solution File No.: 02993 Soln. Date: 12/03/2024 Soln. No.: 00407
Sequential File No.: 02993 File Date: 12/03/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0008
Control Solution %: 0.100% Expires: 05/14/2026
Solution Control Lot: 24180 Bottle No.: 0791

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:19S		
Control 1 EC	0.099%	10:20S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:20S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20S		
Control 2 EC	0.099%	10:21S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22S		
Control 3 EC	0.098%	10:23S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:23S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:23S		

All tests within acceptable tolerance.

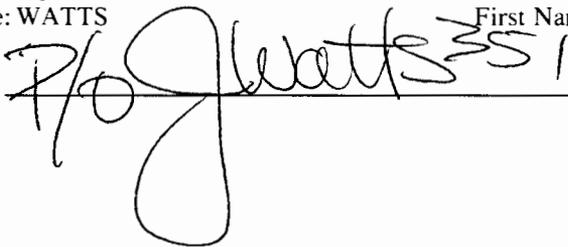
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: 

Badge No.: 351

Date: 12/03/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02960 Calib. Date: 09/16/2024 Calib. No.: 00050
Certification File No.: 02961 Cert. Date: 09/16/2024 Cert. No.: 00044
Linearity File No.: 02962 Lin. Date: 09/16/2024 Lin. No.: 00045
Solution File No.: 02986 Soln. Date: 11/13/2024 Soln. No.: 00406
Sequential File No.: 02986 File Date: 11/13/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0008
Control Solution %: 0.100% Expires: 05/14/2026
Solution Control Lot: 24180 Bottle No.: 0874

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:31S		
Control 1 EC	0.099%	10:32S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:33S		
Control 2 EC	0.099%	10:33S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:33S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:34S		
Control 3 EC	0.098%	10:35S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:36S		

All tests within acceptable tolerance.

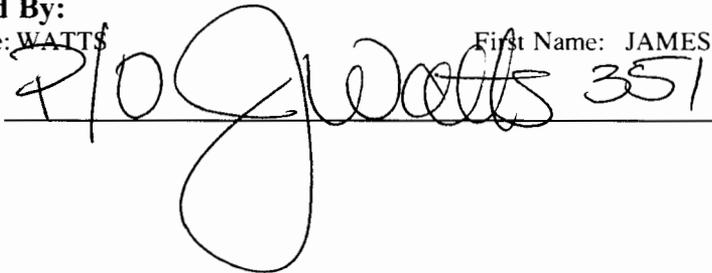
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: 

Badge No.: 351

Date: 11/13/2024

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02960 Calib. Date: 09/16/2024 Calib. No.: 00050
Certification File No.: 02961 Cert. Date: 09/16/2024 Cert. No.: 00044
Linearity File No.: 02962 Lin. Date: 09/16/2024 Lin. No.: 00045
Solution File No.: 02971 Soln. Date: 10/10/2024 Soln. No.: 00404
Sequential File No.: 02971 File Date: 10/10/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0008
Control Solution %: 0.100% Expires: 05/14/2026
Solution Control Lot: 24180 Bottle No.: 0873

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:17D		
Control 1 EC	0.098%	10:18D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:18D		
Control 2 EC	0.096%	10:19D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:19D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		
Control 3 EC	0.097%	10:20D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: 

Badge No.: 351

Date: 10/10/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02911	Calib. Date: 04/23/2024
Certification File No.:	02912	Calib. No.: 00049
Linearity File No.:	02913	Cert. Date: 04/23/2024
Solution File No.:	02957	Cert. No.: 00043
Sequential File No.:	02957	Lin. Date: 04/23/2024
		Lin. No.: 00044
		Soln. Date: 09/10/2024
		Soln. No.: 00402
		File Date: 09/10/2024

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0007
Solution Control Lot:	23200	Expires: 06/05/2025
		Bottle No.: 1228

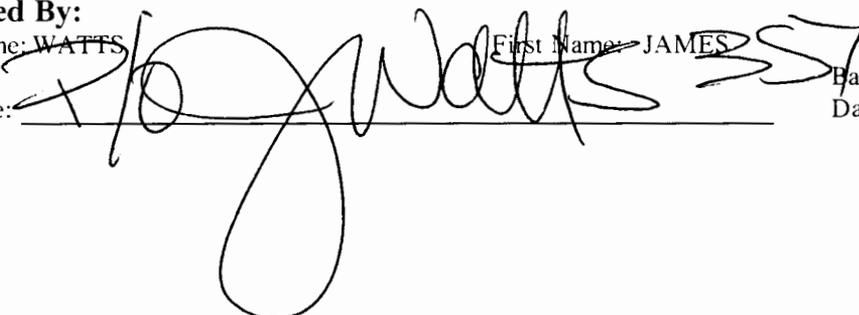
Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:24D		
Control 1 EC	0.098%	09:25D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25D		
Control 2 EC	0.097%	09:26D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:26D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:27D		
Control 3 EC	0.098%	09:28D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:28D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS First Name: JAMES MI: M

Signature:  Badge No.: 351 Date: 09/10/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02911	Calib. Date: 04/23/2024
Certification File No.:	02912	Calib. No.: 00049
Linearity File No.:	02913	Cert. Date: 04/23/2024
Solution File No.:	02948	Cert. No.: 00043
Sequential File No.:	02948	Lin. Date: 04/23/2024
		Lin. No.: 00044
		Soln. Date: 08/15/2024
		Soln. No.: 00401
		File Date: 08/15/2024

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWA S3-0007
Control Solution %:	0.100%		Expires: 06/05/2025
Solution Control Lot:	23200		Bottle No.: 0893

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:57D		
Control 1 EC	0.100%	09:58D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:59D		
Control 2 EC	0.099%	09:59D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00D		
Control 3 EC	0.099%	10:01D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS First Name: JAMES

MI: M

Signature:  351

Badge No.: 351

Date: 08/15/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02911	Calib. Date: 04/23/2024
Certification File No.:	02912	Calib. No.: 00049
Linearity File No.:	02913	Cert. Date: 04/23/2024
Solution File No.:	02946	Cert. No.: 00043
Sequential File No.:	02946	Lin. Date: 04/23/2024
		Lin. No.: 00044
		Soln. Date: 07/22/2024
		Soln. No.: 00400
		File Date: 07/22/2024

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0007
Solution Control Lot:	23200	Expires: 06/05/2025
		Bottle No.: 1051

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:59D		
Control 1 EC	0.100%	09:00D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:01D		
Control 2 EC	0.099%	09:01D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:02D		
Control 3 EC	0.099%	09:03D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

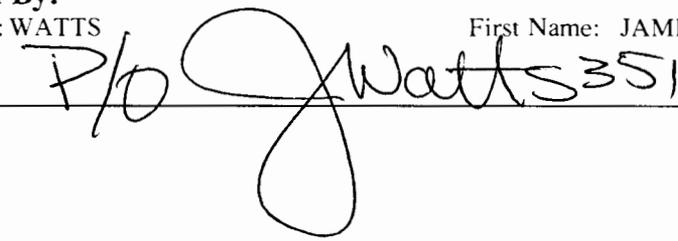
Changed By:

Last Name: WATTS

First Name: JAMES

MI: M

Signature: _____



Badge No.: 351

Date: 07/22/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02911	Calib. Date:	04/23/2024
Certification File No.:	02912	Cert. No.:	00049
Linearity File No.:	02913	Cert. Date:	04/23/2024
Solution File No.:	02943	Lin. Date:	04/23/2024
Sequential File No.:	02943	Lin. No.:	00044
		Soln. Date:	06/28/2024
		Soln. No.:	00399
		File Date:	06/28/2024
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0007
Solution Control Lot:	23200	Expires:	06/05/2025
		Bottle No.:	1233

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:14D		
Control 1 EC	0.099%	07:15D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:16D		
Control 2 EC	0.099%	07:17D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:17D		
Control 3 EC	0.098%	07:18D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Set J W 352

Badge No.: 352

Date: 06/28/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02911	Calib. Date: 04/23/2024
Certification File No.:	02912	Calib. No.: 00049
Linearity File No.:	02913	Cert. Date: 04/23/2024
Solution File No.:	02938	Cert. No.: 00043
Sequential File No.:	02938	Lin. Date: 04/23/2024
		Lin. No.: 00044
		Soln. Date: 06/04/2024
		Soln. No.: 00398
		File Date: 06/04/2024
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0007
Solution Control Lot:	23200	Expires: 06/05/2025
		Bottle No.: 1205

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:18D		
Control 1 EC	0.098%	05:18D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	05:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:19D		
Control 2 EC	0.098%	05:20D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:20D		
Control 3 EC	0.098%	05:21D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCGLINN

First Name: SEAN

MI: M

Signature: _____

P/0 [Signature] 466

Badge No.: 466

Date: 06/04/2024

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02911 Calib. Date: 04/23/2024 Calib. No.: 00049
Certification File No.: 02912 Cert. Date: 04/23/2024 Cert. No.: 00043
Linearity File No.: 02913 Lin. Date: 04/23/2024 Lin. No.: 00044
Solution File No.: 02925 Soln. Date: 05/11/2024 Soln. No.: 00397
Sequential File No.: 02925 File Date: 05/11/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0007
Control Solution %: 0.100% Expires: 06/05/2025
Solution Control Lot: 23200 Bottle No.: 1252

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:56D		
Control 1 EC	0.097%	18:57D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:58D		
Control 2 EC	0.097%	18:58D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:59D		
Control 3 EC	0.098%	19:00D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	19:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:01D		

All tests within acceptable tolerance.

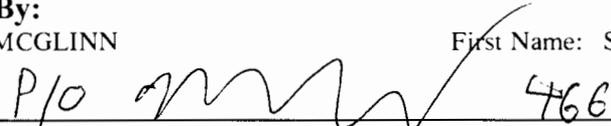
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCGLINN

First Name: SEAN

MI: M

Signature: P/O  466

Badge No.: 466

Date: 05/11/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02911	Calib. Date: 04/23/2024
Certification File No.:	02912	Calib. No.: 00049
Linearity File No.:	02913	Cert. Date: 04/23/2024
Solution File No.:	02914	Cert. No.: 00043
Sequential File No.:	02914	Lin. Date: 04/23/2024
		Lin. No.: 00044
		Soln. Date: 04/23/2024
		Soln. No.: 00396
		File Date: 04/23/2024

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWA S3-0007
Control Solution %:	0.100%		Expires: 06/05/2025
Solution Control Lot:	23200		Bottle No.: 1256

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:56D		
Control 1 EC	0.100%	14:56D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:57D		
Control 2 EC	0.100%	14:58D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:58D		
Control 3 EC	0.100%	14:59D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	14:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUJ P2 - 158 CBH

Changed By:

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: 

Badge No.: 7750

Date: 04/23/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02870	Calib. Date: 08/15/2023
Certification File No.:	02871	Calib. No.: 00046
Linearity File No.:	02872	Cert. Date: 08/15/2023
Solution File No.:	02906	Cert. No.: 00042
Sequential File No.:	02906	Lin. Date: 08/15/2023
		Lin. No.: 00043
		Soln. Date: 11/24/2023
		Soln. No.: 00394
		File Date: 11/24/2023

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWA S3-0008
Control Solution %:	0.100%			Expires:	06/05/2025
Solution Control Lot:	23200			Bottle No.:	1057

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:19S		
Control 1 EC	0.099%	10:20S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20S		
Control 2 EC	0.098%	10:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22S		
Control 3 EC	0.098%	10:23S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.



Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

352

Badge No.: 352

Date: 11/24/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02870	Calib. Date: 08/15/2023
Certification File No.:	02871	Calib. No.: 00046
Linearity File No.:	02872	Cert. Date: 08/15/2023
Solution File No.:	02896	Cert. No.: 00042
Sequential File No.:	02896	Lin. Date: 08/15/2023
		Lin. No.: 00043
		Soln. Date: 11/03/2023
		Soln. No.: 00393
		File Date: 11/03/2023

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWA S3-0008
Control Solution %: 0.100%		Expires: 06/05/2025
Solution Control Lot: 23200		Bottle No.: 1226

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:05S		
Control 1 EC	0.099%	17:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:07S		
Control 2 EC	0.099%	17:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:08S		
Control 3 EC	0.099%	17:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:10S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____


352

Badge No.: 352

Date: 11/03/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02870	Calib. Date:	08/15/2023
Certification File No.:	02871	Cert. Date:	08/15/2023
Linearity File No.:	02872	Lin. Date:	08/15/2023
Solution File No.:	02895	Soln. Date:	11/03/2023
Sequential File No.:	02895	File Date:	11/03/2023
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0008
Solution Control Lot:	23200	Expires:	06/05/2025
		Bottle No.:	1245

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:43S		
Control 1 EC	-.---%	15:44S	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	15:44S	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

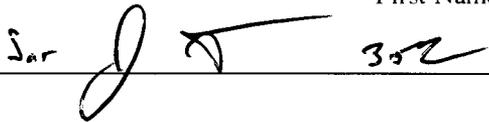
Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____



Badge No.: 352

Date: 11/03/2023

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02870	Calib. Date: 08/15/2023
Certification File No.:	02871	Calib. No.: 00046
Linearity File No.:	02872	Cert. Date: 08/15/2023
Solution File No.:	02884	Cert. No.: 00042
Sequential File No.:	02884	Lin. Date: 08/15/2023
		Lin. No.: 00043
		Soln. Date: 10/11/2023
		Soln. No.: 00391
		File Date: 10/11/2023
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	23200	Expires: 06/05/2025
		Bottle No.: 1249

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:07D		
Control 1 EC	0.100%	08:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08D		
Control 2 EC	0.099%	08:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10D		
Control 3 EC	0.099%	08:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	08:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Set J [Signature] 352

Badge No.: 352

Date: 10/11/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02870	Calib. Date: 08/15/2023
Certification File No.:	02871	Cert. No.: 00046
Linearity File No.:	02872	Cert. Date: 08/15/2023
Solution File No.:	02882	Lin. Date: 08/15/2023
Sequential File No.:	02882	Lin. No.: 00043
		Soln. Date: 09/12/2023
		Soln. No.: 00390
		File Date: 09/12/2023
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	22160	Expires: 05/09/2024
		Bottle No.: 0638

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:00D		
Control 1 EC	0.099%	13:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:01D		
Control 2 EC	0.100%	13:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:02D		
Control 3 EC	0.099%	13:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:04D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

JW
J
352

Badge No.: 352

Date: 09/12/2023

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02811 Calib. Date: 03/16/2023 Calib. No.: 00045
Certification File No.: 02812 Cert. Date: 03/16/2023 Cert. No.: 00041
Linearity File No.: 02813 Lin. Date: 03/16/2023 Lin. No.: 00042
Solution File No.: 02864 Soln. Date: 08/04/2023 Soln. No.: 00388
Sequential File No.: 02864 File Date: 08/04/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0007
Control Solution %: 0.100% Expires: 05/09/2024
Solution Control Lot: 22160 Bottle No.: 0074

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:37D		
Control 1 EC	0.097%	11:38D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	11:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:38D		
Control 2 EC	0.098%	11:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:40D		
Control 3 EC	0.097%	11:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	11:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____



Badge No.: 352

Date: 08/04/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02811	Calib. Date:	03/16/2023
Certification File No.:	02812	Cert. No.:	00045
Linearity File No.:	02813	Cert. Date:	03/16/2023
Solution File No.:	02858	Lin. No.:	00042
Sequential File No.:	02858	Lin. Date:	03/16/2023
		Soln. No.:	00387
		Soln. Date:	07/14/2023
		File Date:	07/14/2023
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0007
Solution Control Lot:	22160	Expires:	05/09/2024
		Bottle No.:	0392

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:13D		
Control 1 EC	0.098%	10:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:15D		
Control 2 EC	0.098%	10:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16D		
Control 3 EC	0.097%	10:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	10:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____



Badge No.: 352

Date: 07/14/2023

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02811 Calib. Date: 03/16/2023 Calib. No.: 00045
Certification File No.: 02812 Cert. Date: 03/16/2023 Cert. No.: 00041
Linearity File No.: 02813 Lin. Date: 03/16/2023 Lin. No.: 00042
Solution File No.: 02843 Soln. Date: 06/21/2023 Soln. No.: 00386
Sequential File No.: 02843 File Date: 06/21/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0007
Control Solution %: 0.100% Expires: 05/09/2024
Solution Control Lot: 22160 Bottle No.: 0147

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:59D		
Control 1 EC	0.099%	09:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:01D		
Control 2 EC	0.099%	09:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	09:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:02D		
Control 3 EC	0.098%	09:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

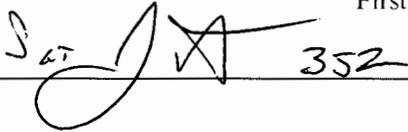
Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

 352

Badge No.: 352

Date: 06/21/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02811	Calib. Date: 03/16/2023
Certification File No.:	02812	Calib. No.: 00045
Linearity File No.:	02813	Cert. Date: 03/16/2023
Solution File No.:	02838	Cert. No.: 00041
Sequential File No.:	02838	Lin. Date: 03/16/2023
		Lin. No.: 00042
		Soln. Date: 05/25/2023
		Soln. No.: 00385
		File Date: 05/25/2023

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWA S3-0007
Control Solution %:	0.100%		Expires: 05/09/2024
Solution Control Lot:	22160		Bottle No.: 0707

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:07D		
Control 1 EC	0.098%	09:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:08D		
Control 2 EC	0.097%	09:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:10D		
Control 3 EC	0.097%	09:11D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Badge No.: 352

Date: 05/25/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02811	Calib. Date: 03/16/2023
Certification File No.:	02812	Calib. No.: 00045
Linearity File No.:	02813	Cert. Date: 03/16/2023
Solution File No.:	02827	Cert. No.: 00041
Sequential File No.:	02827	Lin. Date: 03/16/2023
		Lin. No.: 00042
		Soln. Date: 05/05/2023
		Soln. No.: 00384
		File Date: 05/05/2023
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0007
Solution Control Lot:	22110	Expires: 04/04/2024
		Bottle No.: 0658

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:44D		
Control 1 EC	0.098%	08:45D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:46D		
Control 2 EC	0.099%	08:46D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:47D		
Control 3 EC	0.097%	08:48D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____



352

Badge No.: 352

Date: 05/05/2023

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02811 Calib. Date: 03/16/2023 Calib. No.: 00045
Certification File No.: 02812 Cert. Date: 03/16/2023 Cert. No.: 00041
Linearity File No.: 02813 Lin. Date: 03/16/2023 Lin. No.: 00042
Solution File No.: 02821 Soln. Date: 04/11/2023 Soln. No.: 00383
Sequential File No.: 02821 File Date: 04/11/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0007
Control Solution %: 0.100% Expires: 04/04/2024
Solution Control Lot: 22110 Bottle No.: 0304

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:11D		
Control 1 EC	0.099%	07:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	07:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:12D		
Control 2 EC	0.100%	07:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:14D		
Control 3 EC	0.097%	07:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	07:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

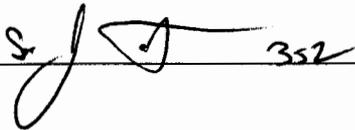
Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____



Badge No.: 352

Date: 04/11/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02754	Calib. Date:	09/28/2022
Certification File No.:	02755	Cert. No.:	00044
Linearity File No.:	02756	Cert. Date:	09/28/2022
Solution File No.:	02803	Lin. No.:	00041
Sequential File No.:	02803	Lin. Date:	09/28/2022
		Soln. Date:	02/07/2023
		Soln. No.:	00380
		File Date:	02/07/2023
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0008
Solution Control Lot:	22110	Expires:	04/04/2024
		Bottle No.:	0542

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:55S		
Control 1 EC	0.102%	07:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:57S		
Control 2 EC	0.102%	07:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	07:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:58S		
Control 3 EC	0.100%	07:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Badge No.: 352

Date: 02/07/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02754	Calib. Date: 09/28/2022
Certification File No.:	02755	Cert. No.: 00044
Linearity File No.:	02756	Cert. Date: 09/28/2022
Solution File No.:	02799	Lin. No.: 00041
Sequential File No.:	02799	Soln. Date: 01/10/2023
		Soln. No.: 00379
		File Date: 01/10/2023
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	22110	Expires: 04/04/2024
		Bottle No.: 0512

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:02S		
Control 1 EC	0.102%	15:03S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	15:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:03S		
Control 2 EC	0.100%	15:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	15:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:05S		
Control 3 EC	0.100%	15:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	15:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Badge No.: 352

Date: 01/10/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02754	Calib. Date: 09/28/2022
Certification File No.:	02755	Calib. No.: 00044
Linearity File No.:	02756	Cert. Date: 09/28/2022
Solution File No.:	02798	Cert. No.: 00040
Sequential File No.:	02798	Lin. Date: 09/28/2022
		Lin. No.: 00041
		Soln. Date: 01/10/2023
		Soln. No.: 00378
		File Date: 01/10/2023

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	21270	Expires: 07/21/2023
		Bottle No.: 0189

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:53S		
Control 1 EC	-.---%	12:53S	22.1°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	12:53S	22.1°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	---:---		
Control 2 EC	-.---%	---:---	N/A	
Control 2 IR	-.---%	---:---	N/A	
Ambient Air Blank	-.---%	---:---		
Control 3 EC	-.---%	---:---	N/A	
Control 3 IR	-.---%	---:---	N/A	
Ambient Air Blank	-.---%	---:---		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

J. Weist 352

Badge No.: 352

Date: 01/10/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02754	Calib. Date:	09/28/2022
Certification File No.:	02755	Cert. No.:	00044
Linearity File No.:	02756	Cert. Date:	09/28/2022
Solution File No.:	02788	Lin. No.:	00041
Sequential File No.:	02788	Soln. Date:	12/13/2022
		Soln. No.:	00377
		File Date:	12/13/2022

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWA S3-0008
Control Solution %:	0.100%			Expires:	07/21/2023
Solution Control Lot:	21270			Bottle No.:	0597

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:32S		
Control 1 EC	0.101%	08:33S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:34S		
Control 2 EC	0.100%	08:34S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:35S		
Control 3 EC	0.099%	08:36S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:37S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Sgt J A 352

Badge No.: 352

Date: 12/13/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02754	Calib. Date: 09/28/2022
Certification File No.:	02755	Calib. No.: 00044
Linearity File No.:	02756	Cert. Date: 09/28/2022
Solution File No.:	02778	Cert. No.: 00040
Sequential File No.:	02778	Lin. Date: 09/28/2022
		Lin. No.: 00041
		Soln. Date: 11/21/2022
		Soln. No.: 00376
		File Date: 11/21/2022

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWA S3-0008
Control Solution %: 0.100%		Expires: 07/21/2023
Solution Control Lot: 21270		Bottle No.: 0185

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:14S		
Control 1 EC	0.101%	09:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	09:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16S		
Control 2 EC	0.100%	09:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	09:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:17S		
Control 3 EC	0.100%	09:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	09:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

[Handwritten Signature] 352

Badge No.: 352

Date: 11/21/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02754	Calib. Date: 09/28/2022
Certification File No.:	02755	Calib. No.: 00044
Linearity File No.:	02756	Cert. Date: 09/28/2022
Solution File No.:	02760	Cert. No.: 00040
Sequential File No.:	02760	Lin. Date: 09/28/2022
		Lin. No.: 00041
		Soln. Date: 10/24/2022
		Soln. No.: 00375
		File Date: 10/24/2022

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	21270	Expires: 07/21/2023
		Bottle No.: 0641

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:56D		
Control 1 EC	0.099%	08:57D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:57D		
Control 2 EC	0.100%	08:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	08:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:59D		
Control 3 EC	0.099%	09:00D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____



352

Badge No.: 352

Date: 10/24/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02695	Calib. Date:	04/26/2022
Certification File No.:	02696	Cert. Date:	04/26/2022
Linearity File No.:	02697	Lin. Date:	04/26/2022
Solution File No.:	02747	Soln. Date:	09/06/2022
Sequential File No.:	02747	File Date:	09/06/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0007
Solution Control Lot:	21090	Expires:	03/17/2023
		Bottle No.:	0144

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:15D		
Control 1 EC	0.100%	08:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:16D		
Control 2 EC	0.100%	08:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:17D		
Control 3 EC	0.099%	08:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	08:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Sgt JWA 352

Badge No.: 352

Date: 09/06/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02695	Calib. Date: 04/26/2022
Certification File No.:	02696	Calib. No.: 00043
Linearity File No.:	02697	Cert. Date: 04/26/2022
Solution File No.:	02735	Cert. No.: 00039
Sequential File No.:	02735	Lin. Date: 04/26/2022
		Lin. No.: 00040
		Soln. Date: 08/08/2022
		Soln. No.: 00372
		File Date: 08/08/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0007
Solution Control Lot:	21090	Expires: 03/17/2023
		Bottle No.: 0090

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:21D		
Control 1 EC	0.101%	12:22D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:22D		
Control 2 EC	0.100%	12:23D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	12:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:24D		
Control 3 EC	0.101%	12:25D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:25D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

S₆T JWE 352

Badge No.: 352

Date: 08/08/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02695	Calib. Date: 04/26/2022
Certification File No.:	02696	Calib. No.: 00043
Linearity File No.:	02697	Cert. Date: 04/26/2022
Solution File No.:	02729	Cert. No.: 00039
Sequential File No.:	02729	Lin. Date: 04/26/2022
		Lin. No.: 00040
		Soln. Date: 07/14/2022
		Soln. No.: 00371
		File Date: 07/14/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0007
Solution Control Lot:	21090	Expires: 03/17/2023
		Bottle No.: 0016

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:07D		
Control 1 EC	0.100%	14:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:08D		
Control 2 EC	0.101%	14:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	14:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:10D		
Control 3 EC	0.101%	14:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Badge No.: 352

Date: 07/14/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02695	Calib. Date: 04/26/2022
Certification File No.:	02696	Calib. No.: 00043
Linearity File No.:	02697	Cert. Date: 04/26/2022
Solution File No.:	02725	Cert. No.: 00039
Sequential File No.:	02725	Lin. Date: 04/26/2022
		Lin. No.: 00040
		Soln. Date: 06/22/2022
		Soln. No.: 00370
		File Date: 06/22/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0007
Solution Control Lot:	21090	Expires: 03/17/2023
		Bottle No.: 0208

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:54D		
Control 1 EC	0.100%	10:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	10:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:56D		
Control 2 EC	0.100%	10:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	10:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:57D		
Control 3 EC	0.101%	10:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Sgt J [Signature] 352

Badge No.: 352

Date: 06/22/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02695	Calib. Date:	04/26/2022
Certification File No.:	02696	Cert. Date:	04/26/2022
Linearity File No.:	02697	Lin. Date:	04/26/2022
Solution File No.:	02714	Soln. Date:	05/23/2022
Sequential File No.:	02714	File Date:	05/23/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0007
Solution Control Lot:	21090	Expires:	03/17/2023
		Bottle No.:	0092

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:34D		
Control 1 EC	0.102%	07:35D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:35D		
Control 2 EC	0.101%	07:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	07:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:37D		
Control 3 EC	0.100%	07:38D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	07:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Badge No.: 352

Date: 05/23/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02633	Calib. Date: 11/16/2021
Certification File No.:	02634	Calib. No.: 00042
Linearity File No.:	02635	Cert. Date: 11/16/2021
Solution File No.:	02689	Cert. No.: 00038
Sequential File No.:	02689	Lin. Date: 11/16/2021
		Lin. No.: 00039
		Soln. Date: 04/14/2022
		Soln. No.: 00367
		File Date: 04/14/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	21270	Expires: 07/21/2023
		Bottle No.: 0323

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:34D		
Control 1 EC	0.101%	13:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:35D		
Control 2 EC	0.101%	13:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:36D		
Control 3 EC	0.100%	13:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Badge No.: 352

Date: 04/14/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	02633	Calib. Date: 11/16/2021
Certification File No.:	02634	Calib. No.: 00042
Linearity File No.:	02635	Cert. Date: 11/16/2021
Solution File No.:	02679	Cert. No.: 00038
Sequential File No.:	02679	Lin. Date: 11/16/2021
		Lin. No.: 00039
		Soln. Date: 03/14/2022
		Soln. No.: 00366
		File Date: 03/14/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0008
Solution Control Lot:	21090	Expires: 03/17/2023
		Bottle No.: 0088

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:23S		
Control 1 EC	0.101%	07:24S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	07:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:25S		
Control 2 EC	0.101%	07:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:26S		
Control 3 EC	0.100%	07:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	07:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:28S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Sgt JAS 352

Badge No.: 352

Date: 03/14/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02633	Calib. Date:	11/16/2021
Certification File No.:	02634	Cert. No.:	00042
Linearity File No.:	02635	Cert. Date:	11/16/2021
Solution File No.:	02669	Lin. No.:	00038
Sequential File No.:	02669	Lin. Date:	11/16/2021
		Soln. No.:	00039
		Soln. Date:	02/24/2022
		File Date:	02/24/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0008
Solution Control Lot:	21090	Expires:	03/17/2023
		Bottle No.:	0089

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:51S		
Control 1 EC	0.100%	08:52S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	08:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53S		
Control 2 EC	0.100%	08:53S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:54S		
Control 3 EC	0.100%	08:55S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

Sgt JWA 352

Badge No.: 352

Date: 02/24/2022

Calibrating Unit

New Standard Solution Report

Equipment

Location: Alcotest 7110 MKIII-C
 CHERRY HILL TWSP. P.D.

Calibration File No.:	02633	Calib. Date:	11/16/2021	Calib. No.:	00042
Certification File No.:	02634	Cert. Date:	11/16/2021	Cert. No.:	00038
Linearity File No.:	02635	Lin. Date:	11/16/2021	Lin. No.:	00039
Solution File No.:	02659	Soln. Date:	01/28/2022	Soln. No.:	00364
Sequential File No.:	02659	File Date:	01/28/2022		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWA S3-0008
Control Solution %:	0.100%			Expires:	03/17/2023
Solution Control Lot:	21090			Bottle No.:	0030

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:09S		
Control 1 EC	0.102%	08:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10S		
Control 2 EC	0.102%	08:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	08:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:12S		
Control 3 EC	0.101%	08:13S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	08:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

See J AT 352

Badge No.: 352

Date: 01/28/2022

Calibrating Unit New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: CHERRY HILL TWSP. P.D.
Serial No.: ARUM-0043
Calibration File No.: 02633 Calib. Date: 11/16/2021 Calib. No.: 00042
Certification File No.: 02634 Cert. Date: 11/16/2021 Cert. No.: 00038
Linearity File No.: 02635 Lin. Date: 11/16/2021 Lin. No.: 00039
Solution File No.: 02654 Soln. Date: 01/03/2022 Soln. No.: 00363
Sequential File No.: 02654 File Date: 01/03/2022
Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0008
Control Solution %: 0.100% Expires: 03/17/2023
Solution Control Lot: 21090 Bottle No.: 0036

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:38S		
Control 1 EC	0.101%	09:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40S		
Control 2 EC	0.100%	09:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41S		
Control 3 EC	0.100%	09:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: Sgt J AS 352

Badge No.: 352

Date: 01/03/2022

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0043
Location:	CHERRY HILL TWSP. P.D.	
Calibration File No.:	03055	Calib. Date: 06/06/2025
Certification File No.:	03056	Calib. No.: 00053
Linearity File No.:	03057	Cert. Date: 06/06/2025
Solution File No.:	03085	Cert. No.: 00047
Sequential File No.:	03085	Lin. Date: 06/06/2025
		Lin. No.: 00048
		Soln. Date: 09/10/2025
		Soln. No.: 00422
		File Date: 09/10/2025

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWA S3-0007
Control Solution %:	0.100%		Expires: 10/08/2026
Solution Control Lot:	24370		Bottle No.: 0914

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:38D		
Control 1 EC	0.099%	09:39D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:39D		
Control 2 EC	0.099%	09:40D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41D		
Control 3 EC	0.099%	09:42D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WATTS First Name: JAMES

MI: M

Signature: _____



Badge No.: 351

Date: 09/10/2025